

Evaluating sound quality in hearing aids with reference test audiograms

CARSTEN DAUGAARD, SØREN L. JØRGENSEN, CHRIS V. JØRGENSEN, SØREN V. LEGARTH AND NICK V. ZACHAROV

DELTA Technical-Audiological laboratory, Edisonvej 24, 5000 Odense C, Denmark

DELTA, SenseLab Venlighedsvej 4, 2970 Hørsholm, Denmark

SUMMARY

In the draft of the IEC 60118-15 standard a set of reference test audiograms are described. These audiograms are defined in order to give a common set of fittings for hearing aids, exposed to broadband measurements.

The audiograms also provide a fine basis for the purpose of evaluating the perceived sound quality from various fitting strategies in hearing aids.

Evaluating sound quality involves creating a number of sound stimuli to evaluate the performance of the fitted hearing aids. By defining and recording sound stimuli from sound scenarios expected to be challenging to hearing aids, as many sound attributes as possible are elicited.

For the evaluation of sound quality, descriptive analysis, a method known from the food industry, was applied. For sound evaluation a panel of normal hearing trained assessors has been used.

Results from the test indicate that differences between the hearing aids fitted with the standard audiograms are clearly audible for a number of sound attributes.

INTRODUCTION

In recent years, open fitted hearing aids with relatively low gain have been a commercial success. Although these undoubtedly provide the basic benefits of hearing aids; level and frequency dependent amplification, which in turn eases the listening effort as well as provide a better speech understanding in noisy situations, they will change the perceived sound from that of the un-amplified ear. In most situations this coloration is desirable at least for the speech understanding, but how does it affect the perceived quality of the sound from the hearing aid?

In order to investigate sound quality across different hearing aids, a reproducible and yet realistic setting of the instruments are needed. Since the fitting algorithm is an important part of a hearing aid today a natural place to start is to fit to a predetermined audiogram. To preserve objectivity, and avoid unintentional bias the collection of data from the sound evaluation needs to be performed in a structured and objective manner. In this article a method for preparing and evaluating the hearing aids is presented.

METHOD

A hearing aid is a very complex sound processor with several partly independent factors affecting the quality of the sound. The choice of hardware will affect the sound quality, as well as the number of algorithms which are enabled in the instrument. Where the hardware and to some extent the fitting settings are stationary, some algorithms i.e. noise suppression add a time-variant element to the case. This increases the complexity of the evaluation and thus demands for a careful selection of sound stimuli to exercise all the realistic combinations of features in the hearing aid.

The sound scenarios for this test were selected from common experience with typical hearing aid challenging events, like traffic noise, at a mall and TV sound. Also scenarios including speech perception were used (Dantale Samsøe story, recording of a 3 persons meeting). Other more inventive and perhaps more selective stimuli could have been presented but the chosen set seems to cover the most obvious scenarios. The selected sound scenarios can be found in table 1.

Stimuli no.	Stimulus name:	English title:	Original recording
1	DANTALE, Samsøehistorien	DANTALE, Samsøe History	Stereo/CD
2	Pausesnak, overvejende kvinder	Pause talk by mainly women	Sound Field
3	Musik: Jazz, sangerinde	Music with female Jazz singer	Stereo/CD
4	“Møde”, 1 mand, 2 kvinder	Meeting, 1 man, 2 women	Sound Field
5	Supermarked	Supermarket	Sound Field
6	Keyboard tasteri	Typing on PC keyboard	Sound Field

Table 1: List of sound scenarios for testing the hearing aid sound reproduction.

Finding the right adjustment for the hearing aids is not as simple a task as it appears to be at a first look. Traditionally, when evaluating hearing aids these are fitted to the user, and the user is asked to answer a questionnaire. Typically, this inventory covers benefits and limitations of the user’s new hearing aids.

Since the fitting is individual, a comparison of the instruments performance rather than the effect from the instrument on the user is difficult to obtain. Historically, in evaluation of hearing aid coupler measurements either a full on gain setting or a reference test gain (RTG) setting has been applied. While the full on gain was an easy technical fix point with all trimmers and volume control in max, the RTG was designed as a technically well defined setting bringing the hearing instrument in a realistic user setup. However, since the initial fitting of a hearing aid has been an increasingly more integral part of the hearing aid, technically defined settings are not able to account for all the possibilities in the fitting software.

One approach to align the hearing aid fittings is to use the adjustment possibilities in the fitting software to reach the same insertion gain (IG) or coupler gain for all hearing aids to be compared. But to match all the IG curves completely will be troublesome and to keep control over the setting of other features in the hearing aid could prove difficult. The clear advantage of this approach of course is that no frequency coloration between the hearing aids appears. Differences in other attributes are not blurred i.e. by a dominating treble. Another matter is what target to aim for when matching the IG curves? A number of generic fitting prescriptions still exist, but will the performance of the hearing aid be reliable when it is forced to emphasis frequency areas that are not natural parts of the strategy for that product?

Rather than evaluating on a complete hearing aid system, another approach could be to focus on a specific part of the hearing aid i.e. the transducer. But although a breakdown in several details of the sound processing in the hearing aid could be very interesting work, it is the sum of the contributions from all parts which results in the sound quality that the user in the end will be listening to. A complex interaction between different algorithms and hardware will only be properly exited in a complex setup where all factors are as realistic as possible.

The third approach that was considered and ultimately selected was to use a predefined audiogram. The audiogram provides the basis for a complete and repeatable setting of the hearing aid, along with the entering of a few other options (i.e. user experience, cognitive capabilities and ear mould type).

In the typical clinical fitting situation an audiogram is applied and the fitting software calculates the settings for the instrument for this particular hearing loss. Although some adjustments also of importance to the sound quality probably will be made in the fine tuning of each hearing aid, it is the initial settings most hearing aid users set out their listening experience with.

Due to the impact of the initial fitting on the sound quality it is fair in this experiment to consider the hearing aid to be a black-box, filling in the audiogram and sound stimuli in one end, receiving sound in a given quality at the other.

This approach is also used as the basis for the IEC 60118-15 draft standard “signal processing in hearing aids.” In this standard a set of “standard audiograms” are proposed, covering a range of 7 hearing losses ranging from a very mild to a very profound hearing loss. A special table includes 3 steeply sloped hearing losses, appropriate for the open fitted hearing aids. [3] The scope of the IEC standard is to obtain level vs. frequency measurements of the standard fitted hearing aids to evaluate hearing aid performance. The measurements commonly referred to as speech gain are carried out with a specific speech-like signal (ISTS) in a coupler. The method is described in the IEC 60318-15 draft-standard. The International Speech Test Signal (ISTS) is developed in Oldenburg Hörzentrum as an artificial speech comprised of phonemes of several languages. [2]

When the scope is to evaluate the performance of hearing aids in terms of sound quality, the standard audiogram approach seems quite straight forward, fitting the hearing aids with one or more of the audiograms, expose the instruments to a selection of sound scenarios and evaluate the outcome. The major drawback from this approach is that the differences in frequency- response as a result of different fitting strategies can be very dominating and that might be a problem when evaluating other attributes of the sound not directly related to this coloration.

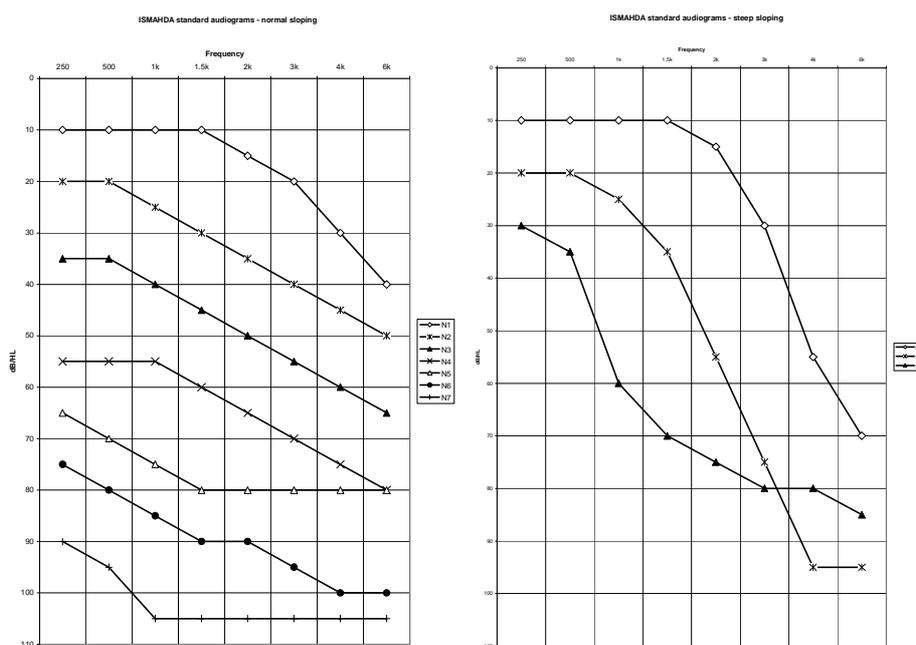


Figure 1: Standard audiograms for hearing aid fitting, as described in IEC 118-15.

With the correctly fitted hearing aids and a good selection of sound scenarios the recordings for the evaluation were made. The fitted hearing aids were placed on a B&K HATS mannequin in the center of a surround sound set-up in an anechoic room. The sound scenarios were played back through the surround sound setup. The resulting mannequin recordings were shortened and presented as stimuli in headphones controlled by an evaluation program running on a computer.

Selecting the assessors for the evaluation was also cause for some consideration. In the field of food sensory a trained assessor panel is used. The panel simply exercises in tasting or smelling very small differences in an attribute for a given product. In similar manner a panel of trained listeners did the evaluation of the recorded stimuli. The seven members of the listening panel had normal hearing, as it is assumed that normal hearing listeners will be at least as capable of evaluating small changes in quality as the slightly hearing impaired listeners who normally wear the products.

The attributes to be assessed were selected by the panel themselves in a so-called word elicitation process, where words associated with listening to a set of the sound stimuli were noted and through a discussion in the panel grouped into a set of attributes characteristic for hearing aid sound perception.

RESULTS

An initial study was made with two different audiograms, the N1 and S1, according to IEC60118-15 draft standard, table 2 and 3. Of course the steeper audiogram shape of S1, compared to N1 gave rise to changed frequency responses in the hearing aid insertion gain, and thus an impression of a high frequency emphasis for recorded stimuli with the S1 fitting. The initial study did not show any particular differences between other attributes from the two stimuli set, and thus only the most radical setting the S1, was used in the subsequent main experiment. This choice was made from the argument that the heavier hearing loss must have the highest probability of eliciting attributes as it simply contributes more to the resulting sound.

From an earlier pilot study we learned that significant differences between hearing aids fitted with a standard audiogram could be perceived, even with non-trained listeners. The main test confirmed this and showed that trained listeners could perform consistently in terms of discriminability, panel agreement, repeatability of judgments and a fair use of the scale for the majority of the tested attributes. However, it must be expected that some attributes are linked to specific sound scenarios, and maybe even to specific hearing aids. Most obvious is the attribute “speech reproduction”, which is only meaningful when evaluated in the two scenarios with understandable speech. The attributes evaluated in the project are found in table 2.

Danish	English
Baggrundsstøj (Svag – Kraftig)	Background noise (Soft – Loud)
Baggrundsstøjens klangfarve (Mørk – Lys)	Background noise tone color (Dark – Bright)
Detaljer (Få – Mange)	Details (Few – Many)
Diskant (Svag – Kraftig)	Treble (Soft – Loud)
Dynamikområde (Lille – Stor)	Dynamic range (Small – Large)

As an example of reading the spider web plot it is seen in figure 2 that the profiles of HA3 and HA4 are quite similar with relatively high scores on “speech reproduction”, “dynamic range” and “details”, while HA5 has a completely different profile with high scores in “treble”, “loudness”, “distortion”, “background noise” and “background noise tone color”. Finally HA2 is seen to have an average scaling on most attributes for this sound scenario.

The spider web plots are drawn for each scenario, so the same profile may not be expected from the same hearing aid, if the different scenarios cause the hearing aid to “react” differently. The plots from this experiment confirm that a certain change of pattern occurs from scenario to scenario, for each hearing aid.

Another way of evaluating the sensory profile is to look at the actual scaling pr. scenario for each hearing aid, and then consider the ranking of hearing aids that are scaled significantly different (see fig. 3). Looking at such plots reveals some interesting points:

- 1) For some attributes one hearing aid seems to “stand out”, with scores that clearly differ from the rest.
- 2) The hearing aids in this test are consistently grouped across sound scenarios.
- 3) For all attributes it is possible to group the hearing aids in 2-3 groups which are scaled significantly different.

Indeed there are significant differences on single attributes for one of the hearing aids. In the attribute “treble” especially HA5 stands out providing much more high frequency gain than the rest across all scenarios, which is particularly obvious in the “meeting” and the “supermarket” situations. This is interesting as there seems to be very little in common between these scenarios. Even more significant is the evaluation of the same hearing aid on the attribute “overload/distortion” where it is evaluated much higher across all scenarios. Other hearing aids also deviate although not that strong. The group comprising of HA1, HA3 and HA4, is performing differently for the “keyboard” stimuli on the attributes “spaciousness”, “resonance”, “background noise”(HA3&HA4) and to some extent “treble”. It is interesting to note that HA1 is scaled significantly higher in background noise for this scenario. This could be explained by looking at the scaling across all scenarios in “background noise”. It seems like the differences between the scaling of the 3 hearing aids decrease in the rather noisy scenarios (supermarket and Jazz), but increase in the quieter scenarios (i.e. “keyboard”, “Dantale” & “meeting”). Therefore it could be speculated that the two hearing aids HA3 and HA4 apply different use of compression/expansion than HA1.

It is interesting to note that the difference in ranking of the hearing aids across scenarios is rather small. It can be seen as a display of robustness of the attributes that they are evaluated uniformly in all scenarios. But if it is assumed, that special scenarios can trigger certain attributes in certain hearing aids, it could also be an indication that the selection of attributes and/or stimuli is not comprehensive enough.

To be able to rank the hearing aids is an important tool in investigating their performance. Looking at the relative placement of a hearing aid on different attributes and in different scenarios makes it possible to investigate the rationale behind the fitting. In some situations the ranking of the hearing aids can be explained by guessing on the behavior of the fitting rationale. As an example: In Background noise for the stimuli “Dantale” and “Meeting” the hearing aid labeled HA1 seems to be more noisy, while in the scenario “girls talk” and “supermarket” the hearing aid HA5 tends to be the noisier. Since the two first mentioned scenarios are closely linked to speech understanding, it could be speculated that HA1 applies much amplification in these scenarios, but in situations that are detected as more noisy, it reduces its amplification, where perhaps HA 5 keeps a rather large gain in all 4 situations, maybe because it detects some speech in all 4 situations.

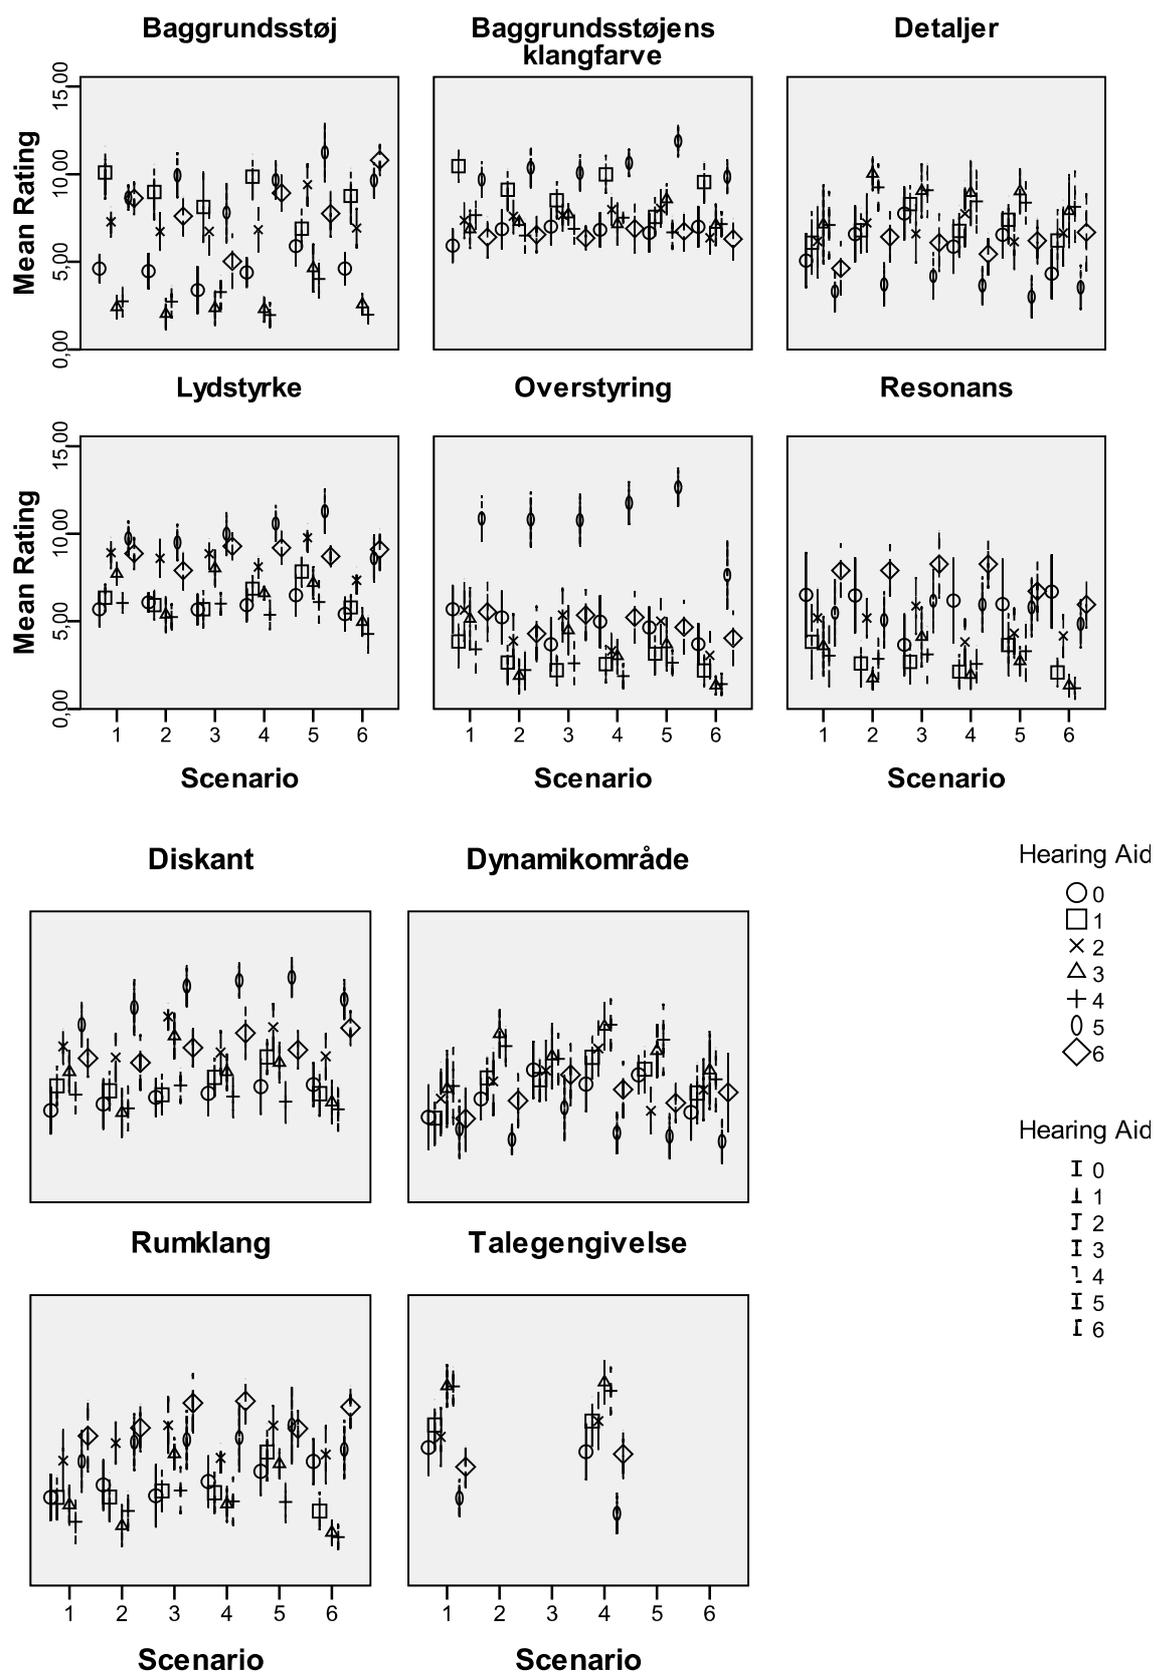


Figure 3: Mean ratings for all hearing aids pr. attribute and scenario. 95% confidence intervals are drawn.

CONCLUSION

A number of hearing aids have been fitted with a standard audiogram and perceptually evaluated. The main result is that hearing aid sound quality can be consistently evaluated with a panel of trained listeners.

Evaluation of all attributes result in groups of significantly differently scaled hearing aids. For the majority of attributes there is a good panel consensus of the judgments. All scenarios seems to elicit the attributes and results in a fairly consistent ranking of groups of hearing aids. The lack of extremely scaled hearing aids for specific scenarios contradict the assumption that some hearing aids react to specific combinations of stimuli and attributes, or indicates that the set of stimuli used for this test has not been selected for that purpose.

The approach of applying standard audiograms does allow for evaluation of a number of attributes, also some not directly connected with the spectral shaping of the fitting process.

The changes in ranking of the hearing aids across attributes and scenarios inspires to explanations related to fitting concepts analogue to the exercise of the technical measurements described in IEC 60118-15, which indicates that the fitting approach also applies nicely to perceptual evaluations.

REFERENCES

- [1] EHIMA: “Background Information on the proposal for testing hearing aids with a speech-like signal”. Version 1.0, (2007).
- [2] Holube, Inga et. al: “Short description of the International Speech Test Signal (ISTS)”
- [3] IEC TC43/WG13: Committee draft 1: IEC60118-15 “Signal Processing in hearing aids”
- [4] Dillon et al.: “Sound quality comparisons of advanced hearing aids”, *The Hearing Journal*, April 2003, vol. 56, no. 4
- [5] Boretski and Launer: “Is there more to fitting than using the right formula ?” chapter 11 from “A Sound Foundation Through Early Amplification”